

AD-A158 071

CRYOGENIC SAMPLE STAGE FOR THE CAMECA IMS-3F ION
MICROSCOPE(U) CORNELL UNIV ITHACA NY BAKER LAB
H T BERNIUS ET AL. 17 JUL 85 TR-14 N00014-80-C-0538

1/1

UNCLASSIFIED


F/G 7/4

NL

END

THUMB

OTIC

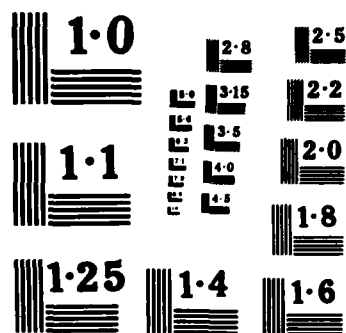

NATIONAL BUREAU OF STANDARDS
MICROCOPY RESOLUTION TEST CHART

(2)

AD-A158 071

OFFICE OF NAVAL RESEARCH

Contract N00014-80-0538

Task No. NRO51-736

TECHNICAL REPORT NO.14

CRYOGENIC SAMPLE STAGE FOR THE
CAMECA IMS-3f ION MICROSCOPE

by

M.T. Bernius, S. Chandra and G.H. Morrison

Prepared for Publication

in

Review of Scientific Instruments

Cornell University
Department of Chemistry
Baker Laboratory
Ithaca, New York 14853

July 17, 1985

DTIC
ELECTE
AUG 15 1985
S B D

DTIC FILE COPY

Reproduction in whole or in part is permitted for
any purpose of the United States Government

* This document has been approved for public release
and sale: its distribution is unlimited

85 8 12 099

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER Technical Report #14	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) CRYOGENIC SAMPLE STAGE FOR THE CAMECA IMS-3f ION MICROSCOPE		5. TYPE OF REPORT & PERIOD COVERED Interim Technical Report
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) M.T. Bernius, S. Chandra and G.H. Morrison		8. CONTRACT OR GRANT NUMBER(s) N00014-80-0538 C
9. PERFORMING ORGANIZATION NAME AND ADDRESS DEPT. OF CHEMISTRY CORNELL UNIVERSITY, ITHACA, NEW YORK 14853		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS NR051-736
11. CONTROLLING OFFICE NAME AND ADDRESS ONR (472) 800 N. Quincy St., Arlington, VA 22217		12. REPORT DATE July 17, 1985
		13. NUMBER OF PAGES 4
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		15. SECURITY CLASS. (of this report) unclassified
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) APPROVED FOR PUBLIC RELEASE: DISTRIBUTION UNLIMITED		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES Summary of work prepared for publication in <u>REVIEW OF SCIENTIFIC INSTRUMENTS</u>		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Secondary Ion Mass Spectrometry (SIMS); Frozen Hydrated Samples. ← Ion Microscopy; Cryogenic; Laboratory Technique; Instrumentation;		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) A liquid nitrogen cooled sample stage for use with the CAMECA IMS-3f ion micro- scope has been designed, built and incorporated into the existing laboratory instru- mentation for SIMS analysis of samples at cryogenic temperatures. This is particu- larly useful for the ion microscopic analysis of frozen hydrated samples (biologi- cals), and the study of sputter and ion yields of materials in a water matrix. The application to semiconductor analysis is being explored. <i>per 1981</i>		

CRYOGENIC SAMPLE STAGE FOR THE CAMECA IMS-3f ION MICROSCOPE

Mark T. Bernius, Subhash Chandra and George H. Morrison
Baker Laboratory of Chemistry
Cornell University,
Ithaca, New York 14853-1301

INTRODUCTION

The ion microscope, based on secondary ion mass spectrometry (SIMS) is a valuable tool for studying the lateral and in-depth elemental (isotopic) distributions in solid samples. To date, analyses were performed on samples that were compatible with the high vacuum environment of the instrument's sample chamber at the ambient temperature of -25°C . This has precluded studies of trace and major elements in group II-VI compound matrices due to their high vapor pressure, and elements in a water matrix, for example.

To this end it was necessary to undertake instrumental research and to design and construct a versatile sample stage completely compatible with standard (room temperature) operations, but with cryogenic capabilities that would allow for the analysis of specialized samples.

MATERIALS AND METHODS

The main features of the standard commercial sample stage can be seen in Fig. 1 and consist of the sample holder, the sample holder mount and the sample stem. The sample holder is a stainless steel piece which serves as a holder for specimens to be analyzed, and facilitates the mechanical transfer of specimens to the sample chamber where it slides onto the mount. The sample holder mount is a stainless steel piece that holds the sample holder during analysis. This mount is fixed to the sample stage, which is attached to the backplate of the sample chamber door and contains a ceramic piece which serves to electrically isolate the sample from ground. This is important because the sample is biased at ± 4500 volts with respect to ground depending on the desired polarity of the secondary ions.

The cold stage had to fulfill the following requirements: 1) To preserve the fine mechanical alignment of the stage with respect to the immersion lens thus allowing the correct secondary ion optical parameters needed by the system. 2) To enable the electrical ± 4500 volt potential to be maintained at the sample holder while all parts outside vacuum and in contact with the body of the instrument to remain at ground potential. 3) To achieve sample temperatures below -150°C during analysis and to maintain it with minimum fluctuation without altering the normal operation of the ion microscope.

The cold stage was therefore designed as shown in Figure 2. It consists primarily of three parts: the bellows arrangement, the cold stem and the liquid nitrogen feedthrough. The first enables the sample stem to fit to the instrument and allows some movement of the stage in the Z- direction. Next is

the cold stem, which consists of a copper top used to insure good thermal conduction silver soldered to a ceramic vacuum break.³ And finally, liquid nitrogen flows through the tube assembly of the sample stem and is in contact with the back side of the copper top.

The sample to be analyzed is held in a special sample holder designed to maximize thermal contact with the cold stage. A temperature sensor is located near the sample for accuracy.

DISCUSSION

The cold stage presented in this work was designed and tested at both room and cryogenic temperatures on the Cameca IMS-3f ion microscope. It is readily adaptable to the existing instrument and is constructed of easily obtainable parts. The stage permits holding a sample specimen at -182°C with liquid nitrogen cooling. Data were obtained for both biological specimens and the copper grid generally used for instrumental alignment under cryogenic conditions. The cold stage presents no more difficulty in operation than the standard (room-temperature) sample stage on the ion microscope.

In addition to biological studies we are exploring other uses for this cold stage on our SMS instrument, such as ion mobility and diffusion studies, analysis of group II-VI semiconductor matrices, and other applications to the material sciences.

Accession For	
NTIS GRA&I	<input checked="checked" type="checkbox"/>
DTIC TAB	<input type="checkbox"/>
Unannounced	<input type="checkbox"/>
Justification	
By	
Distribution/	
Availability Codes	
Dist	Avail and/or Special
A-1	



FIGURES

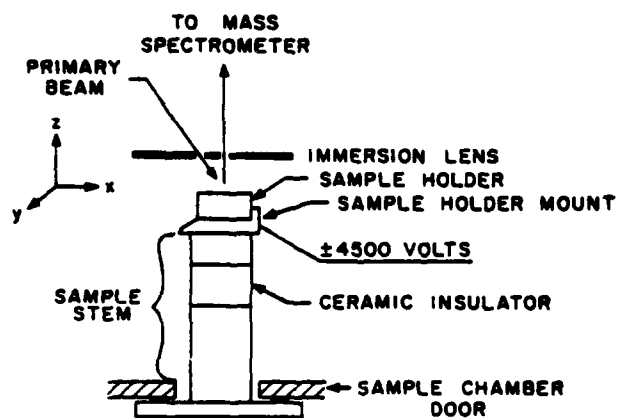


FIG. 1. Schematic of the sample stage system. Shown are the principal areas of interest, the relation of the sample to the immersion lens, and the primary and secondary beam trajectories required for analysis.

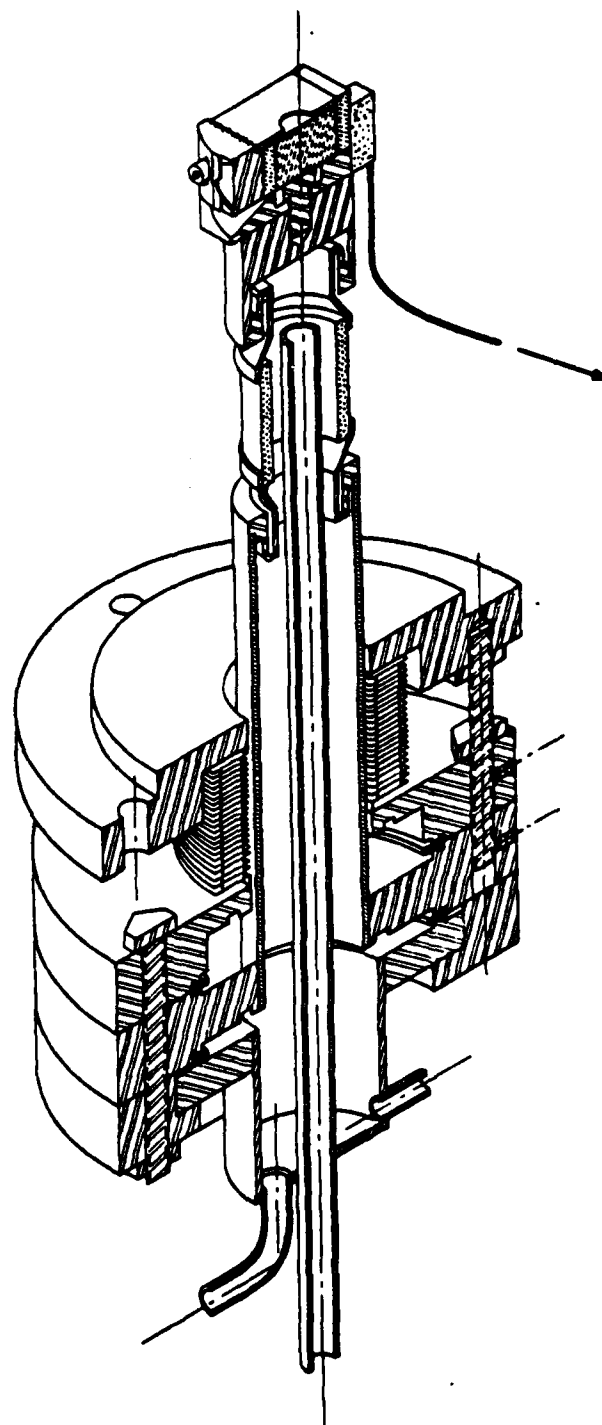


FIG. 2. Isometric-section diagram of the cold stage. Temperature sensor wire is seen leaving the system at the top right (arrow).

TECHNICAL REPORT DISTRIBUTION LIST, GEN

	<u>No. Copies</u>		<u>No. Copies</u>
Office of Naval Research Attn: Code 413 800 N. Quincy Street Arlington, Virginia 22217	2	Dr. David Young Code 334 NORDA NSTL, Mississippi 39529	1
Dr. Bernard Douda Naval Weapons Support Center Code 5042 Crane, Indiana 47522	1	Naval Weapons Center Attn: Dr. Ron Atkins Chemistry Division China Lake, California 93555	1
Commander, Naval Air Systems Command Attn: Code 310C (H. Rosenwasser) Washington, D.C. 20360	1	Scientific Advisor Commandant of the Marine Corps Code RD-1 Washington, D.C. 20380	1
Naval Civil Engineering Laboratory Attn: Dr. R. W. Drisko Port Hueneme, California 93401	1	U.S. Army Research Office Attn: CRD-AA-IP P.O. Box 12211 Research Triangle Park, NC 27709	1
Defense Technical Information Center Building 5, Cameron Station Alexandria, Virginia 22314	12	Mr. John Boyle Materials Branch Naval Ship Engineering Center Philadelphia, Pennsylvania 19112	1
DTNSRDC Attn: Dr. G. Bosmajian Applied Chemistry Division Annapolis, Maryland 21401	1	Naval Ocean Systems Center Attn: Dr. S. Yamamoto Marine Sciences Division San Diego, California 91232	1
Dr. William Tolles Superintendent Chemistry Division, Code 6100 Naval Research Laboratory Washington, D.C. 20375	1		

END

FILMED

10-85

DTIC